



Review: The Development of Infrared Radiation Applications in Medical Field

Qusay Khattab Omer Al-Dulamey

Department of Biophysics, College of Science, University of Mosul, Mosul, Iraq.

qusaykhatab@uomosul.edu.iq

Received Date: 2021/3/27

Accepted Date: 2021/6/27

Abstract

The aim of the study is to demonstrate that infrared imaging can be used as a stand-alone phase in addition to health surveillance and medical evaluation. The advancement of infrared radiation techniques in the medical field in general, and breast cancer applications in particular, necessitates a review of this subject. The medical employ of thermography by infrared began in Germany shortly after 1950, where the single thermal picture of the individuals affected was shown long before (1928). Single Infrared radiation detectors were used at the outset. For a long time, thermal photography cameras soon taken from combat operations operation from low (thermal rather than spatial) resolution, and extraordinarily high product value. In addition, the decrease in laptop hardware value and software value putters. Since about 1980, better medical-suitable technology has been available hot thermocouple scale Fractional Preferential Attachment (FPA) processes have become more reachable, primarily LN2 cooled MCT scanners and then used widely after 2000, and have been widely used in medicine, despite some methodological concerns leading to medical misinterpretation. Individual medical thermal photography processes received certification in 2007, allowing them to be used as medical instruments for thermal measurement. Following European Health Regulations. Other instruments that do not have a CE health certificate are prohibited because photography is not allowed. Measurement functions that aren't used for temperature recording. Qualified medical infrared imaging can be used for a variety of purposes: rheumatology and orthopaedics, female breast region containing sensitive to thermal effort measures thermal radiation, neurology,

cardiac photography (swing-libration vascular thrombosis), lab tests, surgical procedures, and completing body picturing.

Keywords: microwave, spectroscopy, diagnosis, metabolic diseases.

DOI: 10.32894/kujss.2021.168661

مراجعة: تطور تطبيقات الأشعة تحت الحمراء في المجال الطبي

قصي خطاب عمر الدليمي

قسم الفيزياء الحياتية، كلية العلوم، جامعة الموصل، الموصل، العراق.

qusaykhatab@uomosul.edu.iq

تاريخ القبول: 2021/6/27

تاريخ الاستلام: 2021/3/24

الملخص

الهدف من الدراسة هو إثبات أن التصوير بالأشعة تحت الحمراء يمكن استخدامه كمرحلة قائمة بذاتها بالإضافة إلى المراقبة الصحية والتقييم الطبي. يتطلب تقدم تقنيات الأشعة تحت الحمراء في المجال الطبي بشكل عام، وتطبيقات سرطان الثدي بشكل خاص، مراجعة هذا الموضوع. بدأ الاستخدام الطبي للتصوير الحراري بالأشعة تحت الحمراء في ألمانيا بعد فترة وجيزة من عام 1950، حيث تم عرض الصورة الحرارية الوحيدة للأفراد المصابين قبل فترة طويلة (1928). تم استخدام كاشفات الأشعة تحت الحمراء المفردة في البداية. لفترة طويلة، سرعان ما تم التقاط كاميرات التصوير الحراري من العمليات القتالية من دقة منخفضة (حرارية وليست مكانية) وقيمة منتج عالية بشكل غير عادي. بالإضافة إلى ذلك، انخفاض قيمة أجهزة الكمبيوتر المحمول ومضارب قيمة البرمجيات. منذ عام 1980 تقريباً، أصبحت التكنولوجيا المناسبة الطبية الأفضل متاحة على نطاق مزدوج حراري ساخن، أصبحت عمليات المرفق التفضيلي الجزئي (FPA) أكثر قابلية للوصول، خاصة أجهزة المسح الضوئي MCT المبردة LN2 ثم استخدمت على نطاق واسع بعد عام 2000، وقد تم استخدامها على نطاق واسع في الطب، على الرغم من بعض المنهجية. مخاوف تؤدي إلى سوء تفسير طبي. حصلت عمليات التصوير الحراري الطبي الفردي على شهادة في عام 2007، مما يسمح باستخدامها كأدوات طبية لقياس الحراري. اتباع اللوائح الصحية

الأوروبية. يحظر استخدام الأدوات الأخرى التي ليس لديها شهادة صحية CE لأن التصوير غير مسموح به. وظائف القياس التي لا تُستخدم لتسجيل درجة الحرارة. يمكن استخدام التصوير الطبي المؤهل بالأشعة تحت الحمراء لمجموعة متنوعة من الأغراض: أمراض الروماتيزم وجراحة العظام، ومنطقة الثدي الأنثوية التي تحتوي على حساس للجهد الحراري لقياس الإشعاع الحراري، وطب الأعصاب، والتصوير القلبي (تجلط الأوعية الدموية المتأرجح)، والاختبارات المعملية، والإجراءات الجراحية، واستكمال الجسم تصوير.

الكلمات الدالة: الميكروويف، التحليل الطيفي، التشخيص، الأمراض الأيضية.

DOI: 10.32894/kujss.2021.168661

1. Introduction:

Both structural and functional data are used in medical evaluations. X-rays, Doppler effect, light microscopy, and magnetic resonance electron are structural techniques. Practical techniques include electrocardiogram, hematology pressure calculation, electroencephalogram, pulmonary air flow control, and thermography.

Centered on state of the art technology, institutional criteria and protocols, and competent experiments, each diagnostic technique has its own scientific methodology and knowledge base. Each method's diagnostic value is distinguished by its high sensitivity and its precision (ability to diagnose illness).

The first decades of medical infrared thermography were not approved by the medical community due to many shortcomings (Many branched techniques and health agreement, long-standing thermal structures, soft or without computer mechanical operations). The majority of doctors have favored good structural evaluation methods such as X-ray (computer tomography) growth, Doppler effect and magnetic resonance electron. Structural imaging by ill is easier to correlate with function processes, and there is a growing potential for thermal photography in modern medicine.

There is a strong diagnostic accuracy in IR thermography and can therefore classify medical safety rather than single decline from the condition of object medical safety. New

horizons for IR thermography are opened by the recent shift from the conventional medical model a new approach to development (identifying and minimizing hazards) (diagnosis and repair) and improved identification of medicine and helping to support it could be possible.

2. Medicine's Thermal Picture:

In 1956, when patients of breast tumor were tested for asymmetric thermal spots rather than vascularity in IR picture of the breasts, the first recorded use of thermal picturing in medicine field. But some scientific results have been published [2,3] and the first boom in medical field of IR technology [4] was observed in the 1960s, [5] with the firstly process of breast tumor evaluation. In medicine today, thermal picture was not always accepted, primarily due to the early employ. The process, the shallow under-standing of thermal images, and its poorly handled introduction to breast cancer detection in the 1970s [6]. Recently, developments have moved forward a series of activities in a range of related areas to identify the role of IR imaging in medicine [7- 11]. These enhancements an affectation-effective, non-surgical, non-harmful, and friend of injured patients may also evaluate assistance, including the creation of new-production thermal technology, intelligent image treatment viruses, and physiological illness-dependending on thermal image information, in order to determine health status and evaluation.

The region between visible and microwaves in the spectrum is dominated by IR radiation. Based on their temperature, all objects in the universe emit radiation in the thermal area (10^8 - 10^{15} Hz). It gives more strong radiation from the infrared when an object gets warmer, it radiates to a lower one, wave length [9]. IR rays cannot be observed by the sight of a human, Thermal cameras and detectors can, however, be identified. Fig. 1 displays the fine-scale IR spectral band. It is not settled on and can vary the boundaries between various IR spectral regions. The limits that we accept here [12,13].

In general, IR radiation encompasses wavelengths ranging from 0.751 m to 10001 m, among which typical human body emissions measured for diagnostic purposes only occupy a narrow band at wavelengths of 81 m to 121m [14]. The thermal wave is predicated on references [16-19]. This area is also known as the infrared rays of the long-wave IR (LWIR) or body. Thermal infrared (TIR) is another concept generally used in medical IR imaging, which, as

shown in Fig. 1, spans wavelengths. The continuum of electromagnetics and the Thermal Sector roughly 1.41m.

The thermal emission in this region is mainly heat or thermal radiation, hence the thermography symbol. The thermal image is the image of the thermal exposure yield. The near infrared (NIR) region has wavelengths ranging from 0.751 m to 1.41 m. The thermal diffusion we observe in this area is devoid of thermal diffusion [18].

The use of multispectral imaging in medicine has been made possible by new-generation detectors, despite the near and mid-wave thermal locals are not commonly used in human body imaging photography in which both NIR [20] and MWIR (Once of Naval Research Press Release) are detected in various diagnostic cases. In this review, we focus on the issue of thermal imaging in health with the entire thermal spectral region.

3. Understanding of IR Imaging Pathophysiologically Dependent:

Thermal picturing is a biophysiological analysis that screens for minor physiological changes that several disorders, such as contusions, fractures, burns, carcinomas, lymphomas, melanomas, prostate cancer, dermatological diseases, rheumatoid arthritis, diabetes mellitus, deep venous thrombosis (DVT), liver disease, bacterial infections, etc., may trigger. Regional vasodilation, hyperthermia, hyperperfusion, hypermetabolism, and hypervascularization [21-26] are generally associated with these conditions, producing higher-temperature sources of heat. Thermal picturing offers practical data non readily calculated with other tests, various systems like X-radiation traditionally and computed tomography, which mainly gives data on anatomical aspects. Proper employment of thermal pictures therefore is useful in thickness biophysiological expertise its own e-elective understanding. Tumor biological cells as a type of chronic genes modification from a natural biological cell resulted with certain equipped physical effects, such as chemical factors, X-radiation, ultra violet, etc. The imbalanced metabolic activity in all types of cancer cell. It leads to the use of a large dose of blood glucose and results in a high dose of lactate in the blood. In addition, the high metabolic rate of cancer cells causes an increase in local temperature as compared to normal cells. These variables have allowed IR imaging to visualize the anomaly as a viable process. Thermal imaging provides the best complex strange cell information as the

strange cell appears as a soft cell, despite being able to improve rapidly, working it as a high temperature spot in the thermal picture [27,28]. The heat originating from the heat supply and the hematological environment on the surface was quantitated using the between biological cell and Pennes heat link equation [29]. This equation incorporates heat transfer with respect to conduction across the cell, volumetric metabolic thermal production of the cell, and volumetric blood cell pump ratio, the latter of which is influenced by the arterio-venous heat variables [30].

$$K\Delta^2 T - C_b V_b (T - T_a) + qm = 0 \quad (1)$$

where K is conductivity, qm is the tissue's volumetric metabolic rate, $C_b V_b$ is the product of the basic heat power and the blood mass rate per unit volume of biological cell, T is the unidentified tissue temperature, and T_a is the arterial temperature. Theoretically, the emanating heat from the body's surface is measured. We can find the heat style of different internal parts of the body using high thermal imagery by solving the problem of heat movement. In the literature, different states of solving heat transfer in the biological cell equation have been reported [31,32].

While thermodynamics can be used to calculate the thermal radiation of a thermal body, the complexity of biological body-related boundary conditions makes this approach impractical.

A multi-stage analytical repair is biological spectroscopy, including initialization of spacemen, learning the spectrum, repair, and data analysis. One of these steps is hard to find recorded findings in appropriate handling tests [33]. Any molecule has an appropriate infrared spectrum, just like any molecule has its own appropriate vibrational properties. Based on this fact, wave frequency spectroscopy was regarded as a wonderful instrument in the characteristics of multi atomic components. Spectrum comprises a collection of acceptable characteristics such as band position, band depth, and band density with area re-running between bands and peaks to a representation of the multi atomic components of the specimen. These properties may be used in various environments, such as disease states, to acquire functional group information or track molecules. Raman spectroscopy, infrared spectroscopy, and 10^{12} Hz spectroscopy are used in wavelength spectroscopy. Three states allow changes in multi-atomic structure, density, elements, and multi-molecular roles to be expressed in the frequency spectrum bands

and can be resolved with frequency spectroscopy device analyzed. [34,35]. Infrared spectroscopy consists of IR spectroscopy which is far, mid, and close. In biological and medical fields, vibrational spectroscopy has been commonly used. As a simple, precise, non-invasive, cost-effective and operator-independent tool, this analytical system offers distinct data to assess the spectral agent that increases from environmental and pathological conditions. Here, we will discuss infrared analysis in the feature post. The characteristic effect is a recurrent instability between the state of power absorption and dissipation that activates hyper weight gain. In last years, the prevalence of obesity has risen significantly and achieved global epidemic proportions [36,37]. Unhealthy eating patterns, decreased physical activity, Life design improvement, planning, genetic preparation, and youth opposite contribute to an environment that promotes characteristics that allows these ills to be gradually diffused by most older classes [38]. A level of specific body fat aggregation results in the respective improvement of a distinct metabolic virus like insulin confrontation, high glucose sensor, diabetes event, high blood pressure, blood fat adjustment, brain stopping, disease of fatty liver, disease of coronary heart, tumor, and disease of metabolic [39-41]. The advent of metabolic complications leads to genetic and environmental factors, leading to a major medicine and a major economic challenge. Obesity also causes performance to decline due to daily work failures, death ratio and chronic deficiency [42-44] Along with excess expenditure on health care. Early diagnosis is desperately needed, taking into account the non-health implications and medical hazards associated with more fat in the body.

A variety of approaches have been suggested for identifying and characterizing obesity and treating this global burden. The Quetelet Index represents the Body Mass Index (BMI, with unit, in kg/m^2) that is widely used and measured in kilograms converted into meters squared by body weight, like body weight. Additionally, as a body fat code, ultra-weight ($25\text{-}30 \text{ g}/\text{m}^2$) [45] may be unique. The waist circumference (WC) is often used to track central obesity and is measured at a level between the lowest rib and the iliac crest. The risk of disease is determined by a cut-off of 102 cm for men and 88 cm for women with regard to the World Health Organization (WHO). This approach defines the danger of obesity poorly in relation to its systemic difficulties, such as the established issue of measuring bones. As more precise methods for measuring fat lining concentration and body fat spread, magnetic resonance

imaging (MRI) or double energy X-radiation absorption (DEXA) have been used [46]. They are expensive and inaccessible, so other techniques are skin layer thickness, double X-radiation power absorptiometry, bio-electrical resistance, preferred layout, down water calculation, CT scan computed tomography, and close thermal contact. Most of the measured ones are costly and rely on theory and styles without control [47,48]. Because of the above-mentioned advantages, high sensitivity and ease of application. In the field of biophysical and medical articles, infrared wavelength represents the strong energy. In addition, during the appointment method, infrared frequency is recorded as a high that is more suitable to determine the amount of structure change, function, composition and separation of biologically in a relationship component in the specimen.

4. The Interactions Between Matter and Spectroscopy are Based on (Sample Nalyzed):

The several well-known analytical methods that can be used to analyze each form of spaceman, such as solutions, powders, liquids, pastes, and top planes, are reflected in infrared spectroscopy. Since the 1940s, thermal frequencies have proven to be economically beneficial [49].


The very structured increase in thermal wavelength is the beginning of the Fourier-transform formula in the spectrometer unit. This tool uses a coordination scale and potentially defines the Fourier-transformation mechanism as a benefit. Fourier-transform infrared wavelengths have the potential to notice specimens in their fluid state. The accuracy of IR spectra has been significantly improved and the time needed for data acquisition has been minimized [50,51]. Furthermore, with continuous progress in the laptop and light microscope combined with the computer, IR spectroscopy has made more substantial strides. This section abbreviates the essential ideas and their principles related by thermal wavelength and microscopy.

The infrared spectrometer is a system supplied to the infrared wavelength absorption watch that accepts the opening of the multi atom between changing levels of power. The different frequency between changing levels is expressed when the infrared frequency supplement is represented. Notification of infrared radiation absorption and a top peak is

determined. If the absorbed frequency is limited, the infrared frequency and energy are measured as a wavelength function. With infrared study, the motion between strong frequency and curve changes is determined. A chemical infrared wavelength substance is a clone of a multi atomic for its fixed wavelength. Infrared microscopy is a kind of light microscopy, often referred to as IR micro scale spectroscopy, which is useful as a supply that moves infrared light frequencies to recognize the image of the specimen. The infrared microscope has optics like reflective properties that have allowed it to limit the spectrum of all thermal light wavelengths. This system normally consists of an FTIR spectrometer, an optical microscope, and an IR detector. In order to display various parts of the sample. At a single point, a straight array or centered in the plane array point, the infrared assessment will detect thermal light. This allows both topical and wavy information to be processed with respect to the specimen part. The microscope's FT infrared sample is reserved for FT infrared microscopy. The spectrometer's infrared radiation instruments focus on a sample position in the conventional X-radiation process of the light microscope. Upon moving through the sample that produces images of the sample within the restricted area at the microscope, the infrared bands are obtained with topical [52]. A variable aperture is located inside this image plane. The radiation is concentrated on the MCT detector by another condenser after that. Work to imagine the viewing of models clearly, there are also glass targets. Additionally, by moving mirrors in the optical train, the microscope can be transformed from the transmission mode to the reflectance mode.

4.1 Medical thermography and infrared imaging background:

In Germany, the use of infrared thermography for medical targets started in 1952, together with physicist testing, SCHWAMM enhancement of an individual infrared thermometer detector for cascading thermal estimates of individual surface areas of the skin to determine outcomes [53]. Their method has been patented in many countries, including the USA. The individual thermographic health connected with them was noted in 1954. The Deutsche Gesellschaft für Thermographie and Regulationsmedizin e.V. (Deutsche Gesellschaft für Thermographie und Regulationsmedizin e.V., German Field for Thermal Imaging and Health Coordination) continues to be effective today. In the world, both created and tested medical thermographic medical ties. In figure 1, the first medical thermographic system is seen.

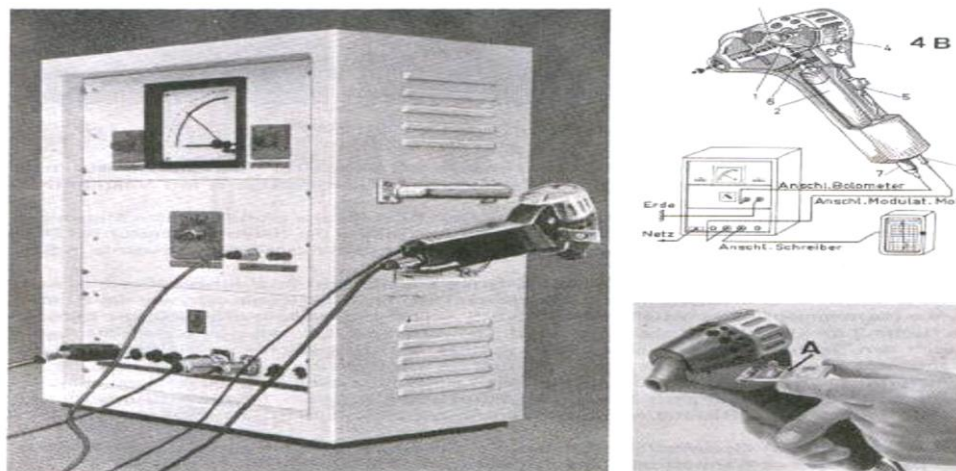

Ultrarot-Strahlungsmesser für Diagnostik und Therapiekontrolle nach Dr. Schwamm-Reeh.

Fig. 1: First thermographic medical unit, developed in 1953 by SCHWAMM and REEH [53].

4.2 Thermography of electronic and LC (liquid crystal) contacts:

The temperature of the skin may also be measured by touch measurement. For unique synthesis as well as plates for two-dimensional region shielding, like encapsulated LC LC, one of the essential thermal measurement thermocouples of electronics as Fig. 2 has been used (liquid cholesterol crystals, Fig. 3) [54-57]. These tools are of historical use where they have been extremely expensive to use as long as thermal cameras have been used and are being installed at an early stage. A range of disadvantages, including contact interference with the restricted section Fig. 2, 3, 4, 5.



Fig. 2: Thermocouples of electronics using for fustigation of medical [53].

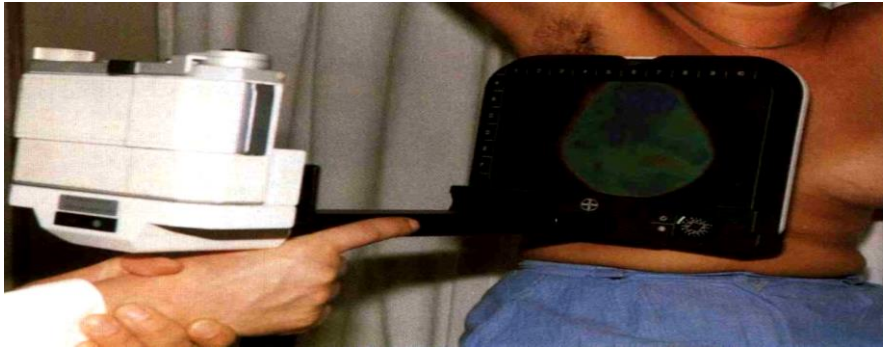


Fig. 3: touch thermos –picture device with fluid [53].

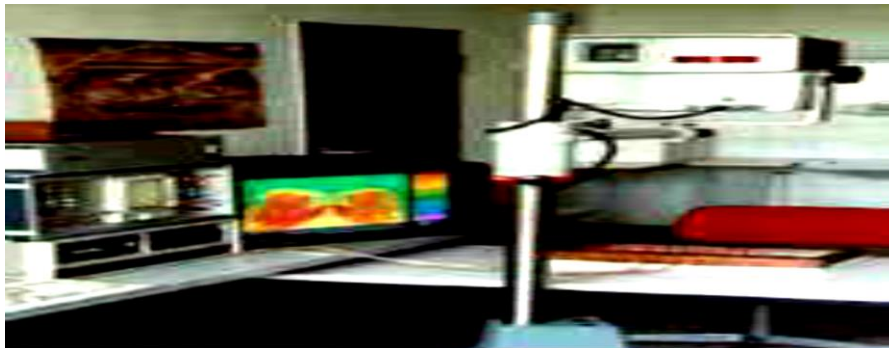


Fig. 4: The iconic 1985 Zeiss Icotherm [69].



Fig. 5: Ther movision cameras which are medically commonly Using [69].

The last 20 years have been characterized by a "explosion" of thermal camera models and manufacturing rather than being used for health objectives. Their software program is growth, as it is historically based on the scanning sensor process. Furthermore, through completely new

technology, individual thermal cameras, non-cooled focus plane array thermocouple cameras, found for health use, facing noise, still pattern, thermal withdrawal and increased instability at the beginning Fig. 6.

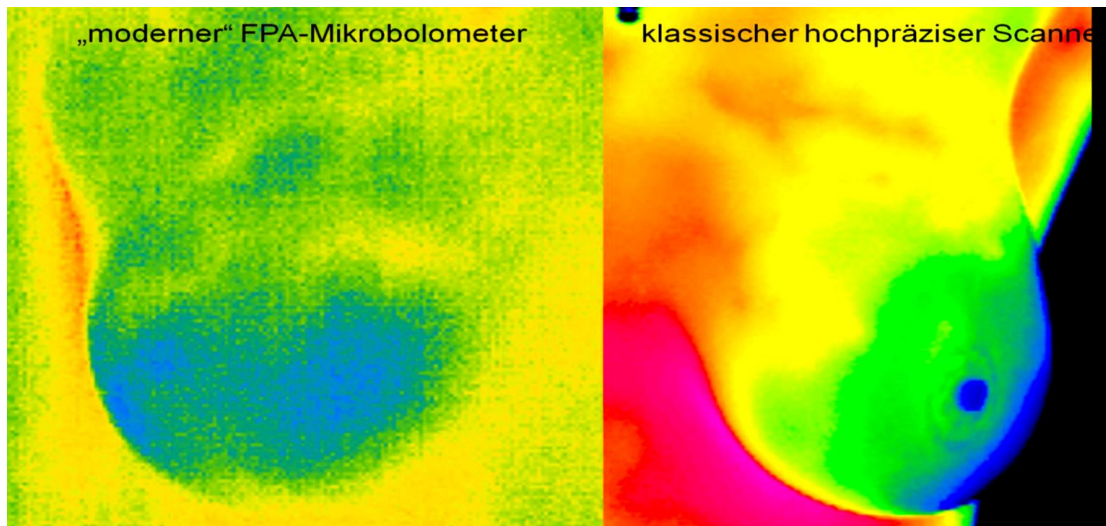


Fig. 6: Compare between cooled scanner sensor and non-cooled focus plane array cameras [55].

Together with advanced microelectronic infrared cameras, significant advantages have recently been achieved. It is a slow recording (1 Hz) and therefore not a real-time imaging system, although it is still necessary to call the cooled MCT scanner the gold standard. Scanners for growth, such as the Jenoptik VarioScan HR Fig. 7 by high analysis and greater stability, multi-sensitivity (better than 30 mK) and thermal drift estrangement, the illumination, penetrating, audio problem and pixel-free images are given.



Fig. 7: The gold standard in medical thermography still today: Jenoptik VarioScan HR [53].

The geometric resolution of even Compared to Megapixel cameras, the new high-resolution thermal cameras are lightweight and arrive to 1×10^6 sensors with resolution development. Thermal cameras are ideal for medical use with High Research Matrix Microbolometer Fig. 8.



Fig. 8: Improved analysis 384x288 Jenoptik VarioCam HR [69].

4.3 Early Cameras for IR:

The early infrared cameras were weak from today's point of view in terms of thermal and geometric resolution and many other things, For example, equilibrium, reproducibility, precise results. Nevertheless, they found that the measured values to be stated were therefore non-contact, dealing with the calculated skin, single employed with (Lawson, 1956) [58]. In the mid-1980s, the researcher Carl Zeiss Oberkochen enhancement noticed heath system at a time span of several years. The Icotherm LN2 cooled MCT scanner Fig. 4, which has sadly highly costs and unaffordable for doctors and clinics. For the most part, since 1983 [59-62] has used all cameras, the more approved watch hot machines (Fig. 5), the medical standard at high time. Body heat is produced and holds the center temperature is provided by metabolism and muscular activity, slow vibration scale (close to 37° degree). The heat disappears from the body rather than the skin, convection, infrared ray, and surface steam when breathing and other processes, depending on both environmental factors and surface outcomes, Fig. 9. with convection (blood drift) and attachment, heat is transported within the organism.

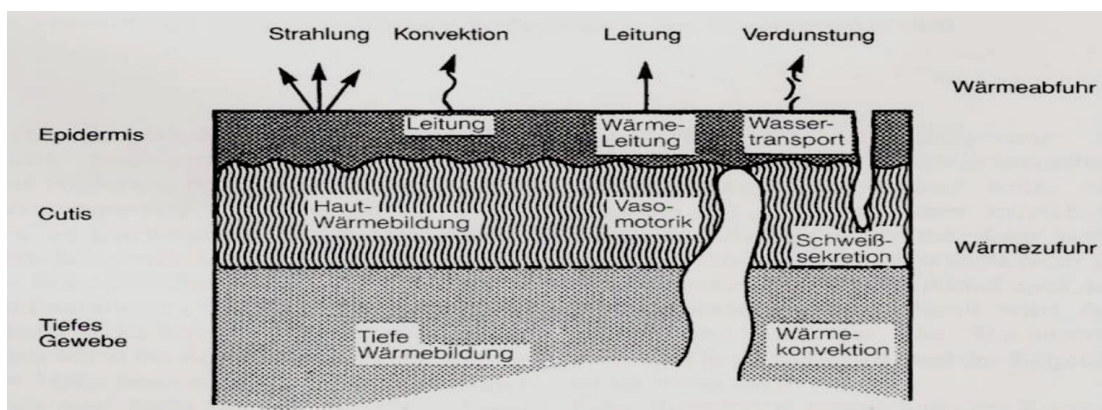


Fig. 9: On the surface of the biological cell, heat loss processes [53].

There is no closely unlearned skin thermal blueprint under administered experimental conditions. That is the acquisition of, well explained by human physiology and pathophysiology, of various synergistic and antagonistic factors and processes. According to the PLANCK law, the dry human surface, nearly built black body [63], is a low thermal wave frequency with a high emission of about 10 μm .

In general, the biological tissue has a "heat stairway" with the highest heat in the head and down the field escorted with the trunk and lowered to the digits of the toes farther on the limbs. There is excess heat that cannot be used while the skin is above the surface for diagnosis (for example, down the breasts section, Fig. 6. Lateral symmetry is the most important feature of the tissue surface temperature design.

5. Diagnostic Infrared Devices Medical Criteria:

5.1 The IR Cameras:

Medically appropriate IR cameras have to follow those specifications. The geometric resolution and temperature analysis of the detector components is similar to 80 $^{\circ}\text{C}$ or more, ideally greater than 50 $^{\circ}\text{C}$. It is important to reliably increase the computed values. It is important to keep the thermal drift in a very narrow range.

Several well-known infrared cameras have recently met these specifications. Individual infrared cameras used for medical computing must be medically CE-certified and certified in



accordance with medical device legislation (in Germany Medizinproduktegesetz) Assessment and data administration

In a data analysis that has the capacity to be used in reading in any external medical program, the measurement information must be sent to the lossless data management system. Characteristic magnitude analysis used by many infrared camera instruments makes their cameras unsuitable for health use. The arrangement of magnitude in health artifacts is extremely constrained and cannot be accomplished by standard software programs supplied by many universally available infrared cameras. All IR applications employed for health objectives must be certified rather than approved in accordance with the regulations on medical devices, similar to IR cameras (in Germany Medizinproduktegesetz).

5.2 Method of data assessment and diagnosis:

The challenging and softer link with the health infrared thermal image sequence is the use of a checked, evaluated and clinically reliable software solution. A CE certifying body must testify to the overall accuracy of the thermal camera movement measurement study via a laptop in the medical infrared external software program. On the basis of precise measurement results, medical IR services will evaluate the data evaluation process and provide recommendations for pathological processes, diagnostic relevance, and therapeutic considerations. Medical Officer.

6. Protocols and Standardization:

Medical infrared thermography has been distinguished by a lack of agreed and mandatory general requirements in recent decades. Before and during the test, these requirements shall cover In the clinic, patient planning and patient management [60].

Similarly, the data management and storage procedures, the use of geometric or other assessment methods, and the statistical techniques used must obey agreed protocols. Unlike the situation in the USA, where there are many competing medical associations and academies, there are only two approved and cooperating infrared thermography medical societies in Europe: the Deutsche Gesellschaft für Thermographie und Regulationsmedizin e.V., referred to above. (DGTR Deutsche Gesellschaft für Thermographie and Control Medicine), which has been in existence.

Health consumers with unsafe approved infrared thermal image systems (referring to health staff, experienced physicians, clinic managers, etc.) are more detrimental to the option of both fines and expenses without harmonious infrared equipment.

7. Medical Infrared Imaging Utilization Developed:

There are several medical areas where it is possible to apply infrared thermography. Just a brief description [64-67]in Rost and Bers [68] and Bers and Sauer can be given here.

A- Whole body Infrared Control picturing - thermal I (Fig. 10)

B- Breast imaging in the infrared (Fig. 11)

C- Divisional infrared photography of some body parts

D- Joint pain, protection of the bone, joint picturing (Fig. 12)

E- Neuroscience F- blood capillary vessels, Infrared venous, arterial and vein picturing Fig. 13.

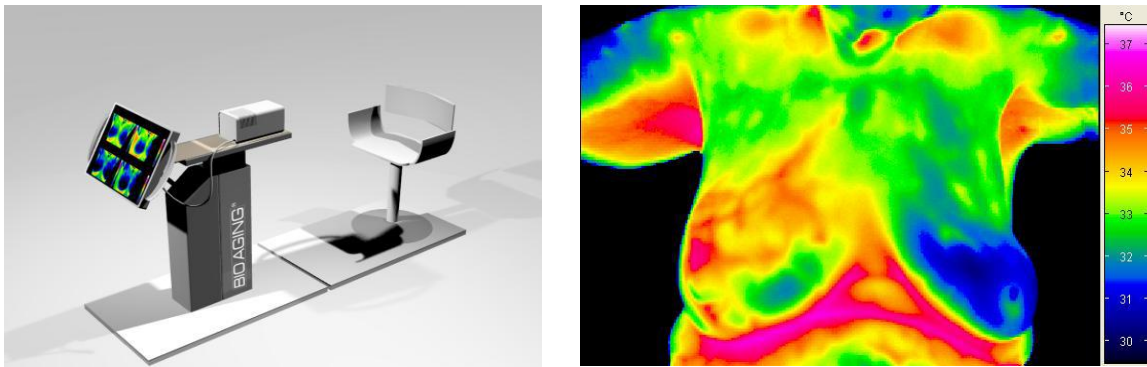


Fig. 10 and 11: Kit for inspection (left) and corresponding image of breast cancer (right) [69].

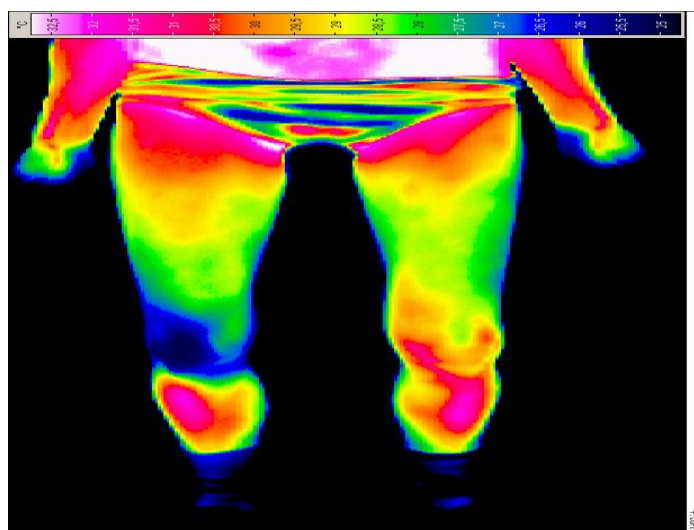


Fig. 12: Gonarthrosis of the left knee [69]

8. Discussion:

In comparison to the concussion of multi-atom bonds, the infrared instrument is a spectroscopic oscillator system that depends on the type of infrared radiation [69-70]. It's a flexible tool for researching biomolecules, cells, and tissues. Structure, positions, and composition have all changed. The effectiveness of this technique has increased in recent years. Scientific researchers have continued to improve medical cases such as tumors and metabolic diseases. Obesity is one of the key causes in tissues such as adipose, liver, and muscle, which is contributing to an increase in the number of dangerous diseases. Unilateral blockages and their ramifications.

It is possible to distinguish molecular modifications as a result of obesity, to understand the multi-atom behavior of the disorder, and to identify reliable spectrum biomarkers that can be used for diagnosis using an infrared device method. Furthermore, to identify the necessary these spectral biomarkers may be used to monitor drugs and their dosages. Applications of spectroscopic and microscopic infrared techniques for characterization. Addresses understanding the diagnosis of magnitude, the metabolism of immensity will resolve the unequal influence of these approaches. Such new methods in the future, light will be added to the estimation of importance in medical applications [71].



Capturing and analyzing infrared images is an excellent technology that enables non-contact, non-invasive biological system investigation, both in preclinical research environments and in patient clinical evaluation. No harmful radiation or other interventions are exposed to the examined specimen, and thus infrared imaging can be considered to be one of the few genuinely green imaging technologies with a great potential for widespread use both in various clinical medicine specialties and in research settings [72].

It is a low-cost, non-radioactive detection tool for the study of skin temperature-related physiological roles called medical infrared thermography that has been used without surgery. Medical thermography has been made a reliable medical measurement instrument by technical advances. A scientific literature search [73] was carried out in order to explore the long-standing assessment and warning value of medical thermography in general medical research. Endocrine glands, repair medicine, musculoskeletal sweats, neural vacillates, tumors and surgery, hover in the area of capillary sweats, we have identified prospective applications. It also helps to know the way Western medical program activities, such as Ayurveda, yoga, and pricked danbees. Coming research must focus on medical thermography testing and clinical modification feasibility testing [35].

9. Conclusions:

Recent advances in medical thermography science were addressed in this review article, with an emphasis on early detection of breast tumors. Regarding the use of infrared cameras, the image processing system, and the pathophysiological nature of electrocardiograms. The aim is to show that infrared imaging can be used as a standalone phase to supplement health surveillance and medical evaluation.

References

- [1] R. N. Lawson, "*Implications of surface temperature in the diagnosis of breast cancer*", Canadian Medical Association Journal, 75, 309 (1962).
- [2] R. N. Lawson and M. S. Chughtai, "*Breast cancer and body temperatures*", Canadian Medical Association Journal, 88, 68 (1963).



-
- [3] R. S. Handley, "*The temperature of breast tumors as a possible guide to prognosis*", Acta Unio Internationalis Contra Cancrum, 18, 822 (1963).
- [4] J. Gershen-Cohen, J. Haberman, and E. E. Brueschke, "*Medical thermography: a summary of current status*", Radiologic Clinics of North America, 3, 403 (1965).
- [5] J. Haberman, "*The present status of mammary thermography*", Ca - A Cancer Journal for Clinicians, 18, 314 (1968).
- [6] J. R. Keyserlingk, P. D. Ahlgren, E. Yu. Belliveau, and M. Y. N., "*Functional infrared imaging of the breast*", IEEE Engineering in Medicine and Biology, 30, (2000).
- [7] M. Anbar, "*Quantitative and dynamic telethermometry-a fresh look at clinical thermos*", IEEE Engineering in Medicine and Biology Magazine, 14(1), 15 (1995).
- [8] J. F. Head, F. M. Wang, C. A. Lipari, and R. L. Elliott, "*The important role of infrared imaging in breast cancer*", IEEE Engineering in Medicine and Biology, 19(3), 52, (2000).
- [9] J. F. Head and R. L. Elliott, "*Infrared imaging: making progress in fulfilling its medical promise*", IEEE Engineering in Medicine and Biology Magazine, 21(6), 80-85, (2002).
- [10] B. F. Jones, "*A reappraisal of the use of infrared thermal image analysis in medicine*", IEEE Transactions on Medical Imaging, 17(6), 1019-1027, (1998).
- [11] J. Keyserlingk, "*Time to reassess the value of infrared breast imaging*", Oncology News International, 6(9), (1997).
- [12] Q. KH. AL-dulamey, A. H. Ismail and Yasir A. Al-Jawwady, "*Testicular Effect of Electromagnetic Radiation on the Function of White Mice*", Iraqi Journal of Veterinary Medicine, 39(2), 48-54 (2015).



-
- [13] Q. KH. AL-dulamey, A. H. Ismail and Yasir A. Al-Jawwady, "*Biophysical Effect of Electromagnetic Radiation on Sex Ratio of White Mice*", International Journal of Advanced Research, 3(6), 1149-1155 (2015).
- [14] Q. KH. AL-dulamey, A. H. Ismail and Yasir A. Al-Jawwady, "*Biophysical effect for electromagnetic radiation on some blood factors of Swiss albino Female mice*". Iraq Journal of Veterinary Medicine, 39(2), 12-14 (2015).
- [15] Q. KH. AL-dulamey, A. H. Ismail and Yasir A. Al-Jawwady, "*Biophysical effect of EMR with 5 GHz on male reproductive system of Mus musculus mice*", Raf.j. Sci, 27(5), Zoology special Issue for the third Scientific Conference of Biology 1-11 (2018).
- [16] Electromagnetic spectrum. Cloudflare WAF Captcha, 11(3), 939 (2001).
- [17] HyperPhysics. Electromagnetic spectrum, hyper physics, 13(4), 578 (2002).
- [18] Infrared Electromagnetic spectrum, Radiation, 22(7), 878 (2002).
- [19] Near, mid & far infrared, California Institute of Technology, 9(4), 333 (2001).
- [20] Thermal imaging, National Research Council, 3(5), 587 (2002).
- [21] J. Whale, "*An introduction to dynamic radiometric thermal diagnostics and dielectric resonance management procedures*", Positive Health, 6(2), 1-24 (2001).
- [22] J. R. Mans eld, M. G. Sowa, J. R. Payette, B. Abdul- rauf, M. F. Stranc, and H. H. "*Mantsch. Tissue viability by multispectral near infrared imaging: a fuzzy C-means clustering analysis*" , IEEE Trans on Medical Imaging, 17(6), 1011-1018 (1998).



-
- [23] Once of Naval Research Press Release, "*Detecting breast cancer with a new algorithm and a multi-spectral infra-red imaging system*", cancer research, 77(15), 342 (2002).
- [24] M. Anbar, "*Clinical thermal imaging today*", IEEE Engineering in Medicine and Biology Magazine, 17(4), 25-33, (1998).
- [25] M. Bale, July-Aug, "*High-resolution infrared technology for soft-tissue injury detection*", IEEE Engineering in Medicine and Biology Magazine, 17(4), 56-59, (1998).
- [26] J. R. Harding, "*Investigating deep venous thrombosis with infrared imaging*", IEEE Engineering in Medicine and Biology Magazine, 17(4),43-46, (1998).
- [27] B. F. Jones and. P. Plassmann. "*Digital infrared thermal imaging of human skin*", IEEE Engineering in Medicine and Biology Magazine, 21(6), 41-48, (2002).
- [28] E. F. J. Ring, "*Progress in the measurement of human body temperature*", IEEE Engineering in Medicine and Biology Magazine, 17(4), 19-24 (1998).
- [29] Szabo T., Fazekas L., Geller L., Horkay, F. Merkely. B. Gyongy, T. and Juhasz-Nagy. May-June, "*A Cardiothermographic assessment of arterial and venous revascularization*". IEEE Engineering in Medicine and Biology Magazine, 19(3), 77- 82, (2000).
- [30] E. Y. K. Ng and N. M. Sudarshan, "*Numerical computation as a tool to aid thermographic interpretation*", Journal of Medical Engineering and Technology, 25(2),53 (2001).
- [31] D. J. Watmough, "*The role of thermographic imaging in breast screening, discussion by C R Hill. In Medical Images:formation, perception and measurement* ", 7th L. H. Gray Conference: Medical Images, 66(22), 142-158 (1976).



-
- H. H. Pennes, "*Analysis of tissue and arterial blood temperature in resting human forearm*", Journal of Applied Physiology, 2, 93-122 (1948).
- [32] Y. K. Ng E. and N. M. Sudarshan, "*Numerical computation as a tool to aid thermographic interpretation*", Journal of Medical Engineering and Technology, 25(2), 53-60 (2001).
- [33] C. L. Chan, "*Boundary element method analysis for the bioheat transfer equation*", ASME J. Heat Transfer, 114, 358-365 (1992).
- [34] T. R. Hsu, N. S. Sun, and G. G. Chen, "*Finite element formulation for two dimensional inverse heat conduction analysis*", ASME J. Heat Transfer, 114, 553-557, (1992).
- [35] F. Severcan, P. I. Haris, "*Vibrational Spectroscopy in Diagnosis and Screening*", Amsterdam: IOS Press, 12-52 (2012).
- [36] F. K. Baloglu, F. Severcan, "*Characterization and differentiation of adipose tissue by spectroscopic and spectral imaging techniques*", In: Szablewski L, editor. Adipose Tissue. Rijeka, Croatia: InTechOpen, intechopen.75156 (2018).
- [37] C. Maiano, O. Hue, A. J. Morin, et al. "*Prevalence of overweight and obesity among children and adolescents with intellectual disabilities: A systematic review and meta-analysis*", Obesity Reviews, 17, 599-611 (2016).
- [38] J. W. Zylke, H. Bauchner, "*The unrelenting challenge of obesity*", Journal of the American Medical Association, 315, 2277-2278 (2016).
- [39] Association, 315, 2277-2278 (2016).



-
- [40] N. K. Kevin, F. C. Vinicius, C. Rodrigo, et al. "***Molecular events linking oxidative stress and inflammation to insulin resistance and β -cell dysfunction***", *Oxidative Medicine and Cellular Longevity*, 2015, 181-643 (2015).
- [41] A. Afshin, M. H. Forouzanfar, M. B. Reitsma, et al., "***Health effects of overweight and obesity in 195 countries over 25 years***", *The New England Journal of Medicine*. 377, 13-27 (2017).
- [42] M. M. Jacome-Sosa, E. J. Parks, "***Fatty acid sources and their fluxes as they contribute to plasma triglyceride concentrations and fatty liver in humans***", *Current Opinion in Lipidology*, 25, 213-220 (2014).
- [43] M. J. Hubler, A. J. Kennedy, "***Role of lipids in the metabolism and activation of immune cells***", *The Journal of Nutritional Biochemistry*, 34, 1-7 (2016).
- [44] T. Andreyeva, R. Sturm, J. S. Ringel, "***Moderate and severe obesity have large differences in health care costs***", *Obesity Research*, 12, 1936-1943 (2004).
- [45] A. Dee, K. Kearns, C. O'Neill, and et al. "***The direct and indirect costs of both overweight and obesity: A systematic review***", *BMC Research Notes*, 7, 242 (2014).
- [46] M. Tremmel, U. G. Gerdtham, P. M. Nilsson, and et al. "***Economic burden of obesity: A systematic literature review***", *International Journal of Environmental Research and Public Health*, 14(4), 435 (2017).
- [47] M. E. Falagas, M. Kompoti, "***Obesity and infection***", *The Lancet Infectious Diseases*, 6, 438e46 (2006).



-
- [48] L. A. Seabolt, E. B. Welch, H. J. Silver, "*Imaging methods for analyzing body composition in human obesity and cardiometabolic disease*", Annals of the New York Academy of Sciences, 1353, 41-59 (2015).
- [49] H. Azizian, J. K. Kramer, S. B. Heymsfield, and et al, "*Fourier transform near infrared spectroscopy: A newly developed, non-invasive method to measure body fat: Non-invasive body fat content measurement using FT-NIR*", Lipids, 43(1), 97-103 (2008).
- [50] A. B. Bernhard, M. A. Santo, V. M. Scabim, et al, "*Body composition evaluation in severe obesity: A critical review*", Advances in Obesity, Weight Management & Control, 4(6), 00113 (2016).
- [51] B. Stuart, "*Infrared Spectroscopy: Fundamentals and Applications*", England: John Wiley & Sons, 15-44 (2004).
- [52] P. R. Griffiths, J. A. Haseth, "*Fourier Transform Infrared Spectrometry*", 2nd Ed., New York: Wiley, 1240-1241 (1986).
- [53] B. Stuart, "*Analytical Techniques in Materials Conservation*", Chichester: Wiley, 113 (2007).
- [54] Z. Movasaghi, S. Rehman, I. Rehman, "*Fourier transform infrared (FTIR) spectroscopy of biological tissues*", Applied Spectroscopy Reviews, 43(2), 134-179 (2008).
- [55] A. Dogan, P. Lasch, C. Neuschl, et al., "*ATR-FTIR spectroscopy reveals genomic loci regulating the tissue response in high fat diet fed BXD recombinant inbred mouse strains*", BMC Genomics, 14, 386 (2013).



-
- [56] F. K. Baloglu, O. Baloglu, S. Heise, et al. "*Triglyceride dependent differentiation of obesity in adipose tissues byFTIR spectroscopy coupled with chemometrics*", Journal of Biophotonics, 10(10), 1345-1355 (2017).
- [57] E. Schwamm, J. Reeh, "*Die Ultrarotstrahlung des Menschen und seine Molekularspektroskopie*", Hippokrates, 24, 737-742 (1953).
- [58] A. Rost, "*Untersuchungen über Kontakt und kontaktlose thermographische Messungen*", Physical medicine and rehabilitation, 21, 610-614 (1980).
- [59] A. Rost, "*Die thermischen Regulationsphänomene und ihre Bedeutung für Diagnose und Prognose*", Thermologische Fachberichte, notamed, Baden-Baden, 20, 314-318 (1983).
- [60] A. Rost, "*Lehrbuch der Regulationsthermographie*", Stuttgart, 333-339 (1994).
- [61] J. L. Fergason, "*Liquid crystals*", Scientific American, 211, 76-85 (1964).
- [62] R. N. Lawson, "*Implications of surface temperature in the diagnosis of breast ledions*", Canadian Medical Association Journal, 75, 309 (1956).
- [63] R. Berz, "*Therapieplanung und Therapiekontrolle mit Hilfe der Thermoregulations diagnostik*", ErfHK, 34, 916-922 (1985).
- [64] R. Berz, "*Das Wärmebild und die Reaktion auf Abkühlung bei jungen gesunden Probanden*", Ärztezeitschrift f Naturheilverfahren, 26, 237-243 (1985).
- [65] R. Berz, "*Thermographie im Wirbelsäulenbereich*", Thermodiagnostik, 1, 20 (1985).



-
- [66] R. Berz, "*Introducing Regulation into Infrared Imaging: ReguVision and MammoVision*", In: Institute of Electronics, Technical University of Lodz (Ed): Proceedings of the 4th National Conference "Termografia i Termometria w Podczerwieni" TTP 2000. Lodz, Poland, 206-212 (2000).
- [67] R. Berz, "*Infrared Regulation Imaging (IRI) – a different approach to health, wellness, and to prevention*", ThermoMed Journal, 16, 49-58 (2000).
- [68] R. Berz, "*MammoVision - A New Approach to Diagnosis and Prevention of Breast Cancer*", In: Benkö I, Kovaczicz I, Lovak I (Eds.): 12th International Conference on Thermal Engineering and Thermogrammetry (THERMO), June 2001, Budapest. Mate, Hungary, 265-272 (2001).
- [69] R. Berz, "*Punktuelle und flächige Brustthermographie im Kontakt- und Infrarotverfahren – eine vergleichende Übersicht*", ThermoMed Journal, 17/18, 29-51 (2002).
- [70] A. Rost, R. Berz, "*Regulationsthermographie nach Rost. In: Augustin M, Schmiedel V (Eds): Leitfaden Naturheilkunde – Methoden, Konzepte und praktische Anwendung*", München (Urban und Fischer), 503-510 (2003).
- [71] R. Berz, H. Sauer, "*Infrarot Regulations Imaging – innovative Funktionsdiagnostik für Früherkennung, Prävention und Problemfälle*", (Infrared Regulation Imaging (IRI) - innovative functional diagnosis for early detection, prevention and solving unclear complaints) ErfHK, 55, 241-250 (2006).
- [72] R. Berz, H. Sauer, "*Comparing effects of thermal regulation tests (cool air stimulus vs. cold water stress test) on infrared imaging of the female breast*", In: Institute of Physics and Engineering in Medicine (Ed): Clinical temperature measurement & thermography. (2007).



- [73] R. Berz, H. Sauer, "*Thermographie und Infrarot Regulations Imaging (IRI)*" , In: Augustin M, Schmiedel V (Eds): Leitfaden Naturheilkunde - Methoden, Konzepte und praktische Anwendung. München (Elsevier, Urban und Fischer), 479-487(2007).